

Instruction for Use

Trade Name: Side Rail Extension

Warning

When using operating table accessories, always pay close attention to the patient. Patients left in the same posture for an extended period of time are at risk for developing nerve paralysis and/or bedsores.

Contraindication/Prohibition

1. This product is only validated for use with Mizuho operating tables.
2. Do not exceed the allowable load specified in **Specifications**, 3. Allowable load. Otherwise the product could break.


Symbol mark for labeling

MD : Medical Device

Specifications

1. Shape

Unit: mm

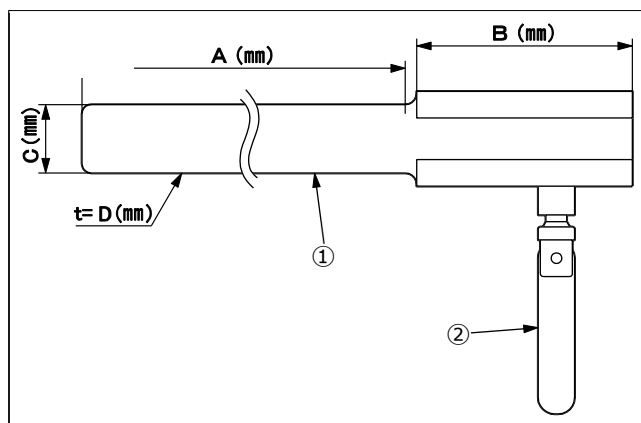

Code No.	Product Description	A	B	C	D
08-115-32	Side Rail Extension *1	220	100	32	9
08-115-70	Side Rail Extension (R2) *2	220	100	25	10

*1 and *2: The size of mountable side rail is different.

2. Weight
1.5 kg
3. Allowable load
Main unit: 25 kg
4. Material
 - ① Rail: Stainless steel
 - ② Fixing handle: Stainless steel

Note: The number corresponds to those used in 1. Shape.


Intended purpose

This is an accessory for the operating table. It is attached to the end of the side rail, allowing attachment of the specified additional accessories.

Intended user

This product is to be used by health care professionals, including but not limited to surgeons, nurses and biomedical technicians.

Instructions for use

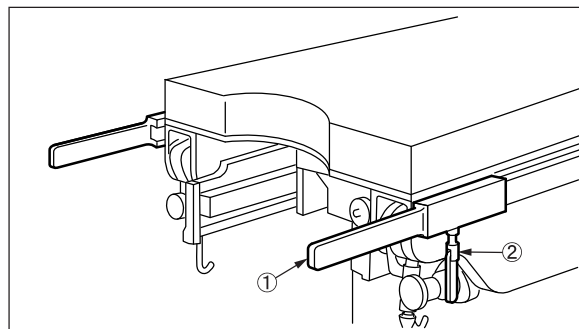

1. Attach the Side Rail Extension① to the side rail of the operating table.
2. Tighten the fixing handle② to fix the Side Rail Extension.
3. Attach the necessary accessories to the Side Rail Extension.

Warning/Caution

1. Warning
Ensure all fixing handles are tight. Loose condition can cause the product to come off or move, which may result in a patient injury.
2. Important caution
 - 2-1. When working with an operating table, take care not to allow this product to make contact or interfere with the tabletop or with other tools and appliances used in combination with this product. Otherwise the product could break.
 - 2-2. For hygiene, be sure to use sterilized drapes on the areas on this product where the patient comes into contact with it.

Storage/Life

1. Do not store the device in high temperatures or in areas with high humidity where the temperature has drastic variations.
2. Service life of this product: 7 years
(Subject to the specified maintenance and inspection and is stored properly.)

Maintenance/Inspection

<By the user>

1. Check before and after use
Check that this product is not damaged or broken before and after each use.
2. Cleaning and disinfection
Wipe off blood, chemicals, contaminants, and other stains with water, and clean the device with gauze or other materials soaked in disinfectants. In addition, use the same disinfectants as the authorized disinfectants on Mizuho's operating table described in the operating table operator's manual.
3. In case of a malfunction
When this product is broken, clearly label the device as "Broken", "Do not use", "Need repair", etc., and contact your local distributor or Mizuho.

<By agents>

Maintenance and inspection can only be carried out by certified agents of Mizuho.

Packing

1 piece per pack

Warranty

MIZUHO Corporation will repair defective parts of this product without charge for one year from the date of delivery/installment except for cases of damage caused by a third party's repair, act of nature, improper use or intentional damage. All other warranty terms and conditions are subject to regulations of MIZUHO Corporation.

Disposal

This device must be disposed of in accordance with local regulations. Please contact your local distributor for proper disposal.

Notice

Any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority in which the user and/or patient is established.



MIZUHO Corporation
3-30-13 Hongo, Bunkyo-ku, Tokyo 113-0033, Japan
<https://www.mizuho.co.jp>



EMERGO EUROPE
Westervoortsedijk 60
6827 AT Arnhem, The Netherlands